

FDR Clinica











Clinical Confidence



Fujifilm is proud to announce our latest high-quality, cost-effective x-ray solution.

The FDR Clinica delivers a user-friendly, smart workflow for busy imaging professionals.





Precision


When your focus is on reducing dose and obtaining excellent image quality, Fujifilm's FDR D-EVO II and FDR ES detectors are the perfect complement to your imaging solution.






Patented ISS capture technology promotes high sensitivity

The FDR Clinica is intended for use with FDR D-EVO II or FDR ES detectors featuring Fujifilm's patented Irradiated Side Sampling (ISS) technology, which positions its capture electronics (TFTs) at the irradiation side, in contrast to traditional detectors. This design significantly suppresses scattering and attenuation of X-ray signals, improving efficiency to produce sharper images at lower doses compared to traditional designs.*





Conventional method ISS system

ISS system reading technology

Optimal Efficiency



The FDR Clinica provides all the advanced features you need to enhance workflow and improve the patient experience.

Utility

New features improve workflow and patient experience.



1 Tilting Wall Stand

A wide variety of exams can be performed using the optional tilting wall stand.

Nonambulatory patients can be easily imaged in the seated position.





2 Dual-reference Rotation

Both top- and center-reference rotation are available in our rotating tray, with automatic connection to the detector. The detector can be rotated while mounted in the tray with no need to remove and remount, greatly reducing handling.





3 Automatic Connection

The detector cable and connector are built into the tray(s), enabling the detectors to be automatically connected when set in the tray. This new function greatly improves efficiency and provides a clean look with no need to manage cabling. The automatic connection to the detector maintains the battery charge so the detector is always ready for wireless use for tabletop, cross table, or wheel chair exams when needed.

Advanced image processing: Dynamic Visualization





Conventional image



New image





Customized image

Fujifilm's renowned digital image processing expertise, including Dynamic Visualization, optimizes image display based on recognition of contrast levels throughout the entire exposure field. The resulting first-up images have outstanding detail and greater window and leveling capability in PACS.

Versatility

FDR Clinica provides flexibility with a wide selection of power ratings to meet your requirements.

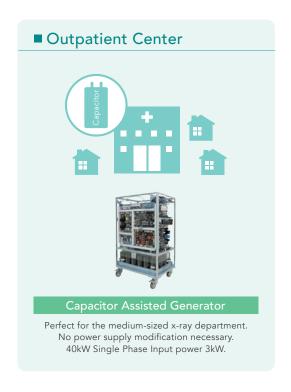

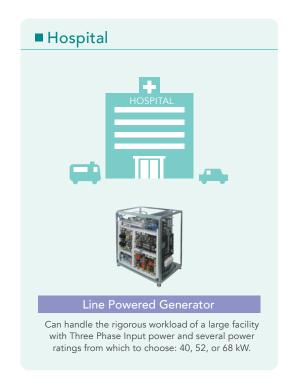

FDR Clinica Specifications

		X-RAY GENERATOR		
	Capacitor Type		Line-power Type	
Product Name	GXR-C40	GXR-40	GXR-52	GXR-68
Output Rating	40 kW	40 kW	52 kW	68 kW
Line Nominal, Phase	110/120VAC, 230VAC, 1Φ	230VAC, 1Ф 400VAC, 480VAC, 3Ф	400VAC, 480VAC, 3Φ	
Line Voltage Range		±10 % (Frequency: 50/60 Hz))	
kV Range	40–150 kV, 1 kV step		/, 1 kV step	
mA Range	10 to 500 mA	10 to 500 mA	10 to 640 mA	10 to 800 mA
Timer Range	0.001 to 10 sec, 38 steps			
mAs Range	0.1 to 500 mAs			
Max. Power Output	500mA@80kV 400mA@100kV 320mA@125kV	500mA@80kV 400mA@100kV 320mA@125kV	640 mA@81 kV 500 m A@104 kV 400 mA@130 kV 320 mA@150 kV	800 mA@85 kV 640 mA@106 kV 500 mA@136 kV 400 mA@150 kV
15A (230VAC, 1Φ) Minimum Breaker Rating 30A (110VAC, 3Φ)		100A (230VAC, 1Φ) 65A (400VAC, 3Φ) 50A (480VAC, 3Φ)	75A (400VAC, 3Ф) 65A (480VAC, 3Ф)	90A (400VAC, 3Ф 75A (480VAC, 3Ф
Anatomical Programs	User-programmable max. 1,280 programs with APR utility software			
Technique Selection	4 point display (kV, mA, Time, mAs)			

Focal Spot Size	0.6/1.5 mm	0.6/1.2 mm
Max. Anode HU	200 kHU	300 kHU
Target Angle	14°	12°
	COLLIMATOR	
E: 1101	B	

COLLIMATOR	
Rectangular	
More than 17x 17 in at 100cm SID	
Min. 2.0 mmAl eq.	
Over 160 LUX at 100 cm SID (Typ. 250 LUX)	
Single LED	
Laser line, Tape measure, Rotating flange	


Continued from the previous page.

Patient Table				
			4-way Floating Tabletop	6-way Elevating Table
Tableto		Longitudinal	39 (±20) in	
Movement Vertical	Transversal	10 (±5) in		
		Travel		11 (22-33) in
		Speed		17 mm/sec
	Vertical	Operating		Motorized movement by footswitch DC-motor (Linear Actuator)
	Bucky	Longitudinal	14 in with standard tray	
		Inherent Filtration	1.2 mmAl	at 100kV
		Max. Patient Weight	660 lbs (300 kg)	
		Size	87 (W) x 30 (D) x 2 (H) in	87 (W) x 32 (D) x 2 (H) in
Bucky Type/Grid Fixed FD 100 cm, 103 lpi, rat		3 lpi, ratio 10:1		
Lock (Brake))		EM Lock, beam sensor on/off	EM Lock, Foot Switch on/off
Center India	cation		Buzzer sound and LED	Transverse center, height center
Dimension/	Weight		87 (W) x 30 (D) x 26 (H) in 330 lbs (150 kg)	87 (W) x 32 (D) x 33 (H) in 573 lbs (260 kg)

Vertical Wall Stand		
Cassette Stroke	Vertical 65 in (17-81 in from floor to Bucky center)	
Bucky Type/Grid	Fixed	FD 150 cm, 103 lpi, ratio 10:1
Lock (Brake)	EM Lock, Switch on/off	
Balance	Counter Weight	
Dimension/Weight	Max. 85 (H) x 26 (W) x 16 (D) in / 264 lbs (120 kg)	

Floor-mounted Tube Stand		
Tube Rotation Angle	±135°	
Tube Stroke	Longitudinal	Max. 87 in
	Lateral	7 in
	Vertical	62 in (17-80 in from floor to focus)
Lock (Brake)	EM Lock, Foot Switch on/off	
Balance	Counter Weight	
Column Rotation	90° step	
Dimension/Weight	91 (H) x 54 (D) x 118 (W) in / 529 lbs (240 kg)	

Dimensions

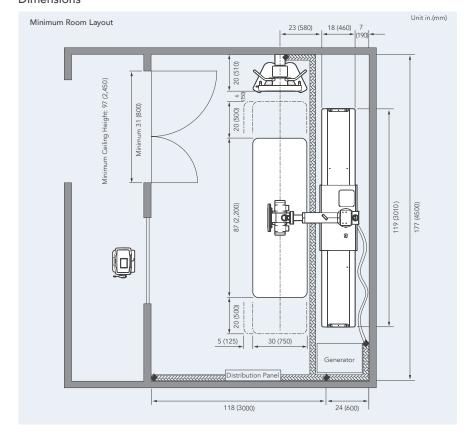

FDR D-EVO II or FDR ES Digital Radiography detectors

FDR D-EVO II or FDR ES G35, G43, C35 and C43 are available for the FDR Clinica. For details, please refer to the brochures.



FDR D-EVO II or FDR ES C35 14x17" and C43 17x17" Cesium models



FDR D-EVO II or FDR ES G35 14x17" and G43 17x17" Gadolinium models

Manufacturer: FUJIFILM Corporation
Specifications are subject to change without notice.

